


# Room 109 - Linac Diagnostic Room

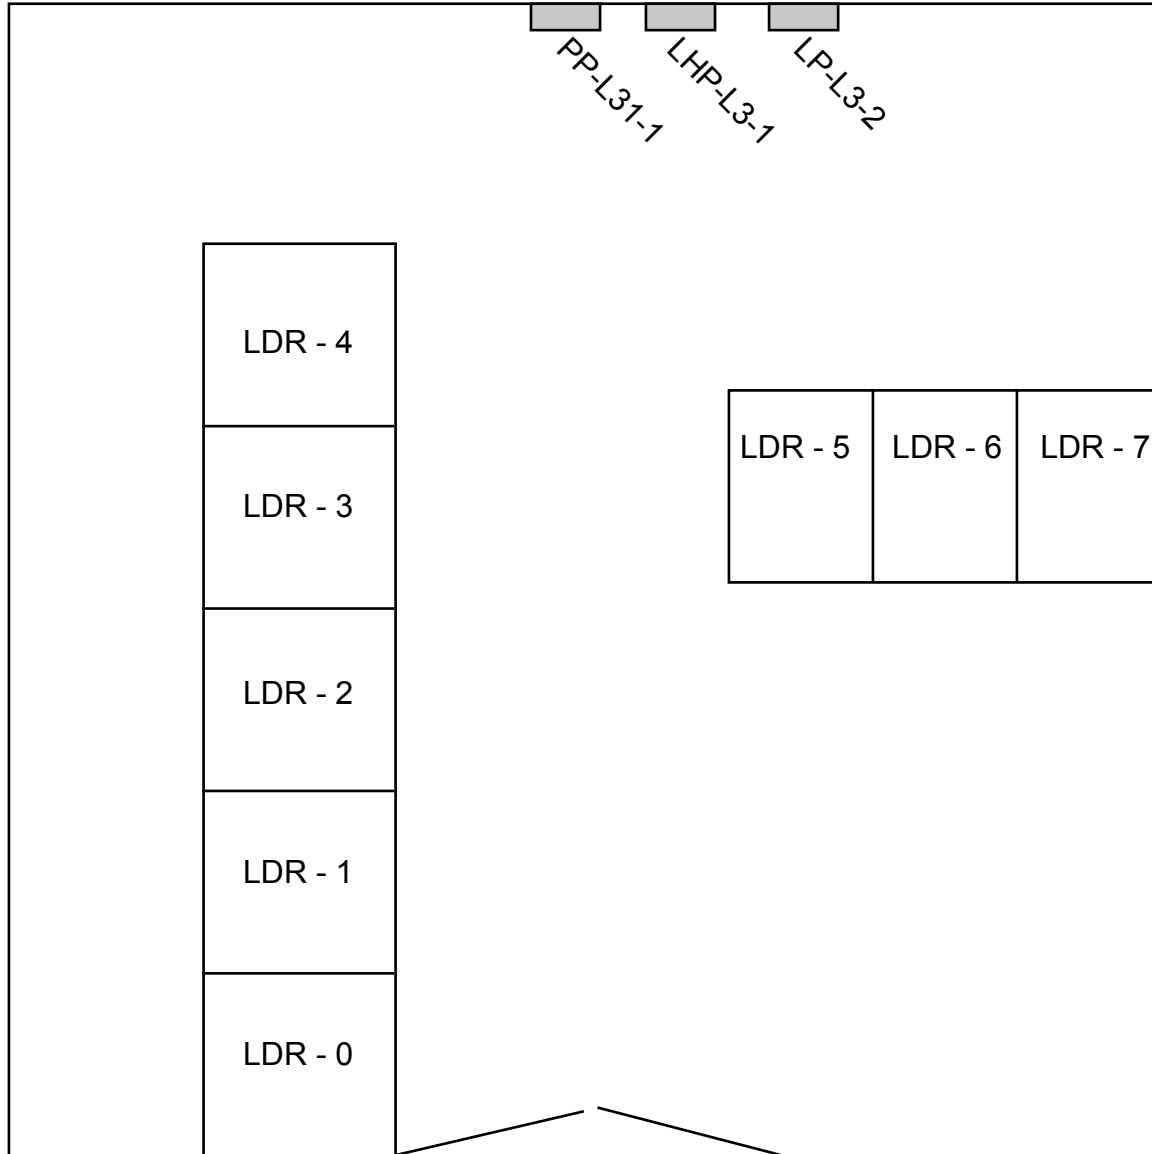

0 - BPM - LNBP05.fnal.gov  
 BPM - LNBP06.fnal.gov  
 BPM - LNBP07.fnal.gov  
 SRM 4  
 8 Channel Rack Monitor

1 - BPM - LNBP08.fnal.gov  
 BPM - LNBP09.fnal.gov  
 32 Channel Sample & Hold  
 062F VME  
 Clock Fan Out Chassis  
 062C VME

2 - SRM 3  
 Beam Phase/Phase  
 Scan Measurement  
 Unknown  
 NIM Crate  
 Phase Detector  
 Module 1 & 2  
 Shay Console

3 - SRM 2  
 32 Channel Sample & Hold  
 NIM Crate  
 L:D0TOR,L: D1TOR,  
 L:D2TOR, L:D3TOR,  
 L:D4TOR, L:D5TOR,  
 L:D73TOR, L:D7TOR,  
 (2) DC Stepping Motor Controllers

4 - SRM 1  
 Glassman HV  
 CATV Modulator

5 - CNS27PC  
 Scope  
 6 - Sun Machine  
 CATV Monitor  
 7 - Computer  
 CAYV Monitor